


Lpm	D50
2	19.768
4	10.057
6	6.773
8	5.116
10	4.116
12	3.446
14	2.965
16	2.603
18	2.32
20	2.094

D50= 2.50
Lpm= 16.67

Work Area
Enter in Red
Answer in Blue
Q-lpm D50
47 1.00

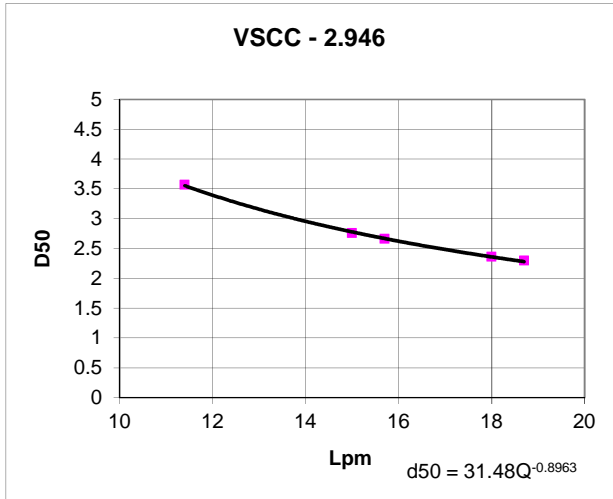


HSE test data

18	2.36
15	2.758
11.4	3.57
15.7	2.66
18.7	2.295

31-Jul-08 Operator: rg
VSCC 2.946 S/N 110308-5
Qs corrected to: BP=760 mm of Hg, T= 20 C
Room BP: 751.3 mm of Hg
RoomTemp: 22.5 C

Work Area
Enter in RED
Answer in BLUE
Q-lpm SP
47 20.7

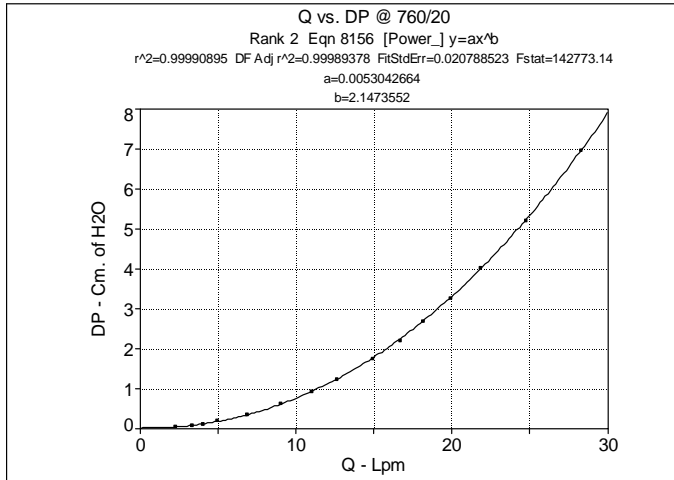

Critical Venturi Number	Reading		Temp. Crit. Vent. C	Qs Lpm	DP DUT	
	Abs. P mm of Hg	Crit. Vent. mm of Hg			Cm of H2O	hPa
# 1	128	22.2	4.944	0.195	0.191	
	174.95	22.3	6.833	0.35	0.343	
	229	22.3	9.005	0.625	0.613	
	279.45	22.2	11.029	0.925	0.907	
	319.8	22.3	12.655	1.225	1.201	
	376.2	22.2	14.917	1.750	1.716	
	419.5	22.4	16.668	2.195	2.153	
	457.2	22.4	18.183	2.685	2.633	
	501.3	22.0	19.930	3.270	3.207	
	549.2	22.1	21.860	4.025	3.947	
	621.15	22.2	24.759	5.200	5.099	
	708.8	22.2	28.280	6.950	6.816	
	#2	203.6	21.8	7.971	0.035	0.034
296.5		21.8	11.698	0.090	0.088	
359.4		21.8	14.222	0.115	0.113	